



Instruction Manual
STANDARD DIGITAL PENETROMER

Product Code

H-5237 & H-5237.5F

**Do not attempt to operate this equipment before reading
and comprehending the manual in all its parts**



Users

MACHINE MANUFACTURERS | DRAUGHTSMEN | OPERATORS | MAINTENANCE WORKERS | ANY OTHERS

REV.	DESCRIPTION	MANAGED	APPROVED	PRODUCT CODE	PAGES	ISSUE DATE
02	Operation Manual	Technical Office	Tech. Manager	B056.M01.EN.02	10	03/2009

Humboldt Mfg. Co.
875 Tollgate Road • Elgin, IL 60123 • 800-544-7220 • www.humboldtmfg.com

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	2/10	03/2009

GENERAL INDEX

Chapter 1	GENERAL INFORMATION
1.01	Warnings
1.02	WARNING and DANGER indications - SIGNS
1.03	Aim of the Instructions Manual
1.04	Modifications and enclosures of the Instructions Manual
1.05	Constructor Identification
1.06	Machine Identification Data
1.07	Usage
1.08	Operators
1.09	Storage
1.10	Transportation and Movement
1.11	Packaging removal
Chapter 2	TECHNICAL CHARACTERISTICS
2.01	General machine description
2.02	Dimension and weight
Chapter 3	GENERAL SAFETY STANDARDS
3.01	General standards
3.02	Machine Safety devices and protection
Chapter 4	INSTALLATION INSTRUCTIONS
4.01	Location
4.02	Handling and movement
Chapter 5	IN FUNCTION - USE
5.01	Machine calibration – Meters - Indicators
5.02	Base spirit level regulation
5.03	Equipping – Sample positioning
5.04	Switching the appliance on
5.05	Test Start Up
5.06	Practical usage example
Chapter 6	MAINTENANCE
6.01	Ordinary Maintenance
6.02	Extraordinary Maintenance
6.03	Authorised maintenance centres
Chapter 7	GUIDE TO RECOGNISING DAMAGE AND ANOMALIES
Chapter 8	SPARE PARTS
Chapter 9	INACTIVITY
Chapter 10	DECOMMISSIONING THE MACHINE

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	3/10	03/2009

Chapter 1 GENERAL INFORMATION

1.01 WARNINGS

The manufacturer does not accept any responsibility for direct or indirect damage to people, things or animals and use of the appliance in different conditions from those foreseen.

The manufacturer reserves the right to make changes to the documentary information or to the appliance without advance notice.

Check the machine responds to the standards in force in the state in which it has been installed.

All operations necessary for maintaining machine efficiency before and throughout use are the operator's responsibility.

Carefully read the entire manual before operating the machine.

It is vital to know the information and limitations contained in this manual for correct machine use by the operator.

Interventions are only permitted if the operator is accordingly competent and trained.

The operator must be knowledgeable about machine operations and mechanisms.

The purchaser must ensure that operators are trained and aware of all the information and clarifications in the supplied documentation.

Even with such certainty the operator or user must be informed and therefore aware of potential risks when operating the machine.

Safety, reliability and optimum performance is guaranteed when using original parts.



Any tampering or modifying of the appliance (electrical, mechanical or other) which has not been previously authorised in writing by the manufacturer is considered abusive and disclaims the constructor from any responsibility for any resulting damage.

All necessary operations to maintain the efficiency of the machine before and throughout use are the responsibility of the user.

1.02 WARNING AND DANGER INDICATIONS - SIGNS

The machine has been designed and constructed according to the current norms and consequently with mechanical and electrical safety devices designed to protect the operator or user from possible physical damage. Residual risks during use or in some intervention procedures on the device are however present. Such risks can be reduced by carefully following manual procedures, using the suggested individual protection devices and respecting the legal and safety norms in force.

This manual includes "Warning" and "Danger" indications in relevant chapters. These indications are shown with the words "Danger" or "Warning" in bold font and uppercase to make them highly visible.

	WARNING	indicates that machine damage could be caused should indications be ignored.
	DANGER	indicates that machine damage and/or injury to the worker could be caused should indications be ignored.

"**DANGEROUS ZONE**" indicates any zone inside or in the proximity of the appliance in which a person is exposed to the risk of injury or damage to health.

1.03 AIM OF THE INSTRUCTIONS MANUAL

This manual has been edited with the aim of providing all machine operators with all the necessary information on installation, use and maintenance from production to scrapping in as comprehensive and clear manner as possible.

All the procedures useful for any foreseeable emergency situations have been listed by the manufacturer and can be verified during use.

Operators, for whom this manual has been written, due to their competence must give instructions or operate the machine themselves.

The instructions manual must be carefully consulted by laboratory or site safety managers, equipment operators and any internal and external maintenance workers.

The manual is integral to the product and refers to this appliance only.

The manual must be safeguarded and always kept near the equipment so that it can be easily consulted whenever necessary.

IMPORTANT: The manual does not substitute the experience and technical training of the worker but must be considered a guide for carrying out its functions.

Furthermore all the norms and rules the operator should be aware of or consult for correct use of the machine and/or test performance can be found in the manual.

This responsibility is entrusted to the installer and Laboratory or Site Manager where the machine is installed.

The Constructor is available to provide further information.

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	4/10	03/2009

1.04 MODIFICATIONS AND ENCLOSURES OF THE INSTRUCTIONS MANUAL

This manual reflects the state at the time of the launch of the machine on its market. If any modifications, improvements or adjustments have been made since machine supply the Manufacturer does not have to intervene on the marketed machine and will not consider the machine or the manual deficient or inadequate.

1.05 CONSTRUCTOR IDENTIFICATION

MATEST SPA
Via Delle Industrie, 25
24048 Treviolo
(Bergamo) Italy
Tel +39 0352055011
Fax +39 0352055055
Email : matest@matest.com
Internet : www.matest.com

1.06 MACHINE IDENTIFICATION DATA

MODEL : B056-01 KIT / S165-01 KIT

PRODUCTION DATA: vedi dichiarazione CE

INSTRUCTIONS MANUAL CODE: B056-01KIT.M01.IT.02

1.07 USAGE

B056-01KIT

This equipment is used to determine a precise value of the consistency of a bituminous sample.

During the test the specimen is vertically penetrated by a standard needle under fixed conditions of load, time and temperature.

S165-01KIT

This equipment is used for determining the content of water at which a ground passes from the plastic to the liquid state by means of the penetration of a cone that freely falls into the specimen.

This appliance is for the exclusive use which it has been conceived for.

Any other use is considered improper and therefore negligent.

Machine use is allowed only in places free from danger of explosion or fire.

During operation check for conditions of danger.

immediately stop the machine should it be working irregularly, and consult the authorised dealer's Sales Service department.

It is the Client's responsibility to verify at the time of installation and use that no conditions of use arise which are different to those indicated.

Refer to the Constructor when in doubt.

1.08 OPERATORS



**DANGER
WARNING**

The use, transportation, installation, maintenance, demolition and disposal of the appliance are only permitted to "QUALIFIED PERSONNEL".
This manual is exclusively aimed at "QUALIFIED PERSONNEL" and contains the necessary information for machine use.

"QUALIFIED PERSONNEL" means people who, due to their training, experience and education, as well as knowledge of the relevant standards, limitations and measures, have been authorised by the "PLANT SAFETY MANAGER" to carry out any necessary activity and are able to recognise and avoid any possible danger.

The manufacturer recommends that the instructions, procedures and recommendations in this manual and the work safety legislation in force be scrupulously adhered to, even with the use of appropriate protection devices (whether individual or part of the machine).

Knowledge and respect of the instructions, safety warnings and danger in this manual are all necessary for installation, operation, management and machine maintenance with a minimal risk.

The "PLANT SAFETY MANAGER" has the following responsibilities and duties:

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	5/10	03/2009

- To know the machine functions, its commands, safety and protection devices, possible dangers of use and all the information in this manual in detail. This knowledge can only be gleaned from detailed reading of this manual.
- To know the safety legislation in force in detail in order to operate the machine
- To recognise the "QUALIFIED PERSONNEL" for transportation, handling, installation, use, maintenance, disposal, etc.
- Correctly train and educate the "QUALIFIED PERSONNEL" before allowing them access to the machine. The personnel must also be exhaustively trained with regards to the machine's protection devices.
- Ensure the machine's safety devices are not tampered with or removed and are checked on a daily basis. Provide the operator appropriate individual protection devices according to the laws in force.
- The constructor is available for clarification, assistance and training and declines all responsibility for damage to things or people resulting from improper, incorrect and negligent use by untrained personnel.

1.09 STORAGE



WARNING

The appliance must be stored and conserved in the original packaging and in a closed environment, protected from atmospheric agents with a minimum temperature of -15C°, and a maximum of +60C° and a maximum humidity of 70%.

1.10 TRANSPORTATION AND MOVEMENT



WARNING

In order to avoid irreparable machine damage, move with care, do not overturn, protect from rain, do not stack, protect the packaging and its contents from bumps and sources of heat.

During transportation and movement it is important to avoid bumps, overloading with other packages, exposure to freezing or heating atmospheric agents, or any other potentially harmful condition to the device, things or people. Machine transportation and movement must be entrusted to Qualified Personnel who can ensure correct movement.



WARNING DANGER

Do not transport or move the product should it be impossible to respect the conditions on the packaging or there be any doubts. Request information from the constructor

1.11 PACKAGING REMOVAL

After removing the packaging check the machine is complete and that there are no visibly damaged parts. DO NOT USE THE MACHINE and refer to the constructor when in doubt.



DANGER

The components used for packaging (plastic bags, polystyrene, nails, screws, wood, etc) must be kept out of reach of children, as they are sources of danger. These components should be placed in the appropriate containers.




WARNING

In order to avoid bumps and overturn adopt the normal and logical precautions. Before disposing of the packaging check all machine components such as accessories, utensils, instructions, documents etc have been removed.


Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	6/10	03/2009

Chapter 2 TECHNICAL CHARACTERISTICS

2.01 GENERAL MACHINE DESCRIPTION

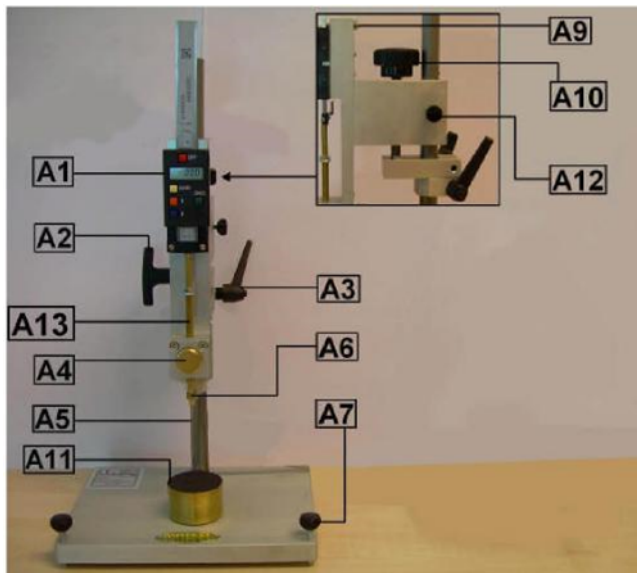

ELECTRONIC METER

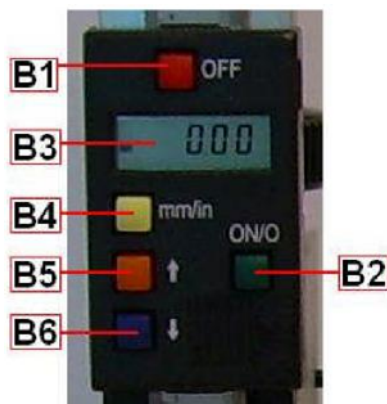

- **A1 -ELECTRONIC METER:**
Measures penetration of the needle or the cone in the sample.
- **A2 - CLAMP :**
Holds the penetrometer in place after positioning the needle or the cone in the intended place.
- **A3 -CLAMP:**
Holds the clamp in place which determines the correct height of the penetrometer for the test to be carried out.
- **A4 - BUTTON:**
When the button is pressed the penetration needle or penetration cone will free fall.
- **A5- PENETRATION NEEDLE OR CONE B056-01 KIT: penetration needle S165-01 KIT: penetration cone**
- **A6 - TIGHTENING SCREW**
Holds the needle or cone in the penetration beam.
- **A7 - KNOBS:**
Level out the instrument.
- **A10 - KNOB:**
Micrometer height regulation of the penetration needle or cone relative to the sample.
- **A11 - CONTAINER:**
Contains the sample to be tested.
- **A12 - KNOB :**
After regulating needle or cone height the tightening screw fixes the penetrometer to the stand, avoiding that it loosens.
- **A13 - PENETRATION BEAM:** the beam containing the penetration needle or the penetration cone where the penetration measurement of the needle or cone in the sample takes place.
- **B1 - OFF BUTTON :** Press this button to switch the electronic meter off (A1).
- **B2 - ON BUTTON :** Press this button to switch the electronic meter on (A1); this button can be also used to reset to zero the value shown on the LCD display regardless of its position.
- **B3 - LCD DISPLAY**
- **B4 - MM/INCHES SWITCHING BUTTON:** Press this button to switch the scale form mm to inches or otherwise
- **B5/B6 - PRE SETTING BUTTONS :** Press and keep on pressing the buttons B5 (for negative values) or B6 (for positive values) to pre-select the height value. The display will start showing the increasing or decreasing value by increasing the speed progressively.

2.02 DIMENSION AND WEIGHT

LENGTH	200 mm
WIDTH	260 mm
HEIGHT	500 mm

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	7/10	03/2009

Chapter 3 GENERAL SAFETY STANDARDS

3.01 GENERAL STANDARDS

To ensure the safety of machine operators:

- Any tampering with the appliance not pre-emptively authorised by the manufacturer exempts the manufacturer from any responsibility for damage caused by or to it.
- The removal or tampering with safety devices entails a violation of the safety standards.
- Machine use is only allowed in areas where there is no risk of explosions or fires.
- Only the original fittings can be used. The use of unoriginal fittings exonerates the manufacturer from all responsibility.
- Check the appliance is in ideal working conditions and that its parts are not worn or faulty before Carry out all necessary maintenance
- Do not wear loose clothing, ties, chains or anything else which could become caught in the frame or other moving parts of the appliance.
- Be aware of the danger of electrical shocks from direct or indirect contact due to unforeseen electrical faults.
- Do not subject the appliance to violent impact.
- Do not expose the appliance to fire, welding sparks or extreme temperatures.
- Do not bring the appliance into contact with corrosive substances.
- Do not wash the appliance with jets of water.
- Check the workspace around the machine is clear from potentially dangerous objects.
- The machine operator must wear appropriate work clothing such as protective glasses, gloves and mask in order to avoid damage from, for example, harmful dust projection. Wear a lower back support when lifting heavy parts. There should be no hanging objects such as bracelets or otherwise, long hair should be protected with relevant precautions, shoes must be appropriate for the type of operation to be carried out.

DURING USE

When operating check there are no conditions of danger. Immediately stop the machine when it is functioning irregularly. Contact the authorised Sales Service department.

- For the operator's safety do not touch any part of the appliance when testing and use the appropriate individual protection devices in order to keep the operator safe.

3.02 MACHINE SAFETY DEVICES AND PROTECTION

DEFINITION: Protections are all the safety measures that consist of the use of specific technical means (repairs, safety devices) to protect people from dangers which cannot be limited reasonably in design.



DANGER

Tampering with the protections or any appliance modification could cause risks to users or other exposed people.
The manufacturer does not assume any responsibility for direct or in direct damage to people, things or animals following tampering with the protections.

Chapter 4 INSTALLATION INSTRUCTIONS

4.01 LOCATION

The equipment must be placed in an ideal position and environment for the use it has been conceived for (laboratory use and protected from atmospheric agents) and that the machine is placed by a qualified operator.

ALLOWED TEMPERATURE:	from +5°C to +40°C
ALLOWED RELATIVE HUMIDITY:	from 30% to 70%
MAXIMUM HEIGHT OVER SEA LEVEL:	1000 m

GENERAL ADVICE

- The machine must be installed in an area which allows ease of access to all parts so that maintenance may be carried out.
- Unauthorised people and objects which could be potential sources of danger must not be permitted in the area surrounding the machine.

Do not position the equipment near instruments or appliances which could produce vibrations.

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	8/10	03/2009

4.02 TRANSPORTATION AND MOVEMENT

These instructions are applicable to the machine assemblers.

Ensure the equipment is correctly supported at the lifting point and that the machine does not slip.

Do not remain in direct line with the application of force and do not allow personnel where there are loads that cannot be adequately supported by mechanical means.

Chapter 5 IN FUNCTION - USE



**DANGER
WARNING**

Before setting the machine in motion it is essential that the Operator and Safety Manager have read the Instructions Manual and understood all parts of the machine and activities linked to it (Risks, Dangers, Functionality, Operation, Protections, Commands, etc.)


5.01 MACHINE CALIBRATION – METERS - INDICATORS

The machine is checked in the factory, using sample equipment periodically checked by officially recognised institutes. These checks cannot guarantee that the machine, meters and indicators will provide accurate values and results conforming to the standards in force in the countries the machine has been installed and used in.

Normally such norms envisage calibration check after every movement. In order to obtain correct values and results it is therefore VITAL that the operator, once the machine has been installed and set up and before official tests, has an officially recognised body check the machine characteristics, its calibration and results/values reliability. The manufacturer is exempt from all responsibility in the case of direct and indirect damage from use of the machine without official approval by the relevant bodies.

5.02 BASE SPIRIT LEVEL REGULATION

Before carrying out the test it is important that the base is placed horizontally. Regulate with the **A7** knobs and check the position in the **B2** spirit level.

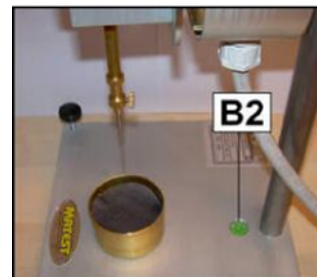

5.03 EQUIPPING – SAMPLE POSITIONING

Put the additional weight, to be chosen from the range supplied with the equipment, on the upper part of the penetration beam the fit additional weight for the execution of the test among those furnished in endowment with the tool

The following calibrated weights are supplied:

- B056-01 KIT: n°1 weight 50g + n°1 weight 100g
- S165-01 KIT: n°1 weight 20g

Raise the position of the beam of the **A1** meter until the end.

Press **A4** and raise the **A13** penetration beam until it hits the penetrometer and release the button in order to hold the beam.

Insert the needle or the cone **A5** into the penetration beam **A13** and lock it by means of the tightening screw **A6**.

Ensure the **A2** clamp is tightened.

Open the knob on the **A3** clamp and position it at such a height so the penetration needle or cone is positioned 3-4 mm above the hypothetical surface of the sample.


After doing so close the knob firmly and do not open it for the rest of the test.

Open the knob on the **A2** clamp and gradually move the penetrometer until it rests under the **A3** clamp. Turn the penetrometer so that it corresponds to the point of the needle, with the centre of the instrument base.

Tighten the **A2** clamp. Throughout the test it is possible to loosen it every time the needle or cone needs to be moved laterally, without altering its height.

Position the **A11** container which has already been filled with the sample to be tested on the base of the penetrometer, more or less centred with the tip of the **A5** penetration needle.

Consult the UNI- EN1426 standard for the correct procedure in order to fill the **A11** container.

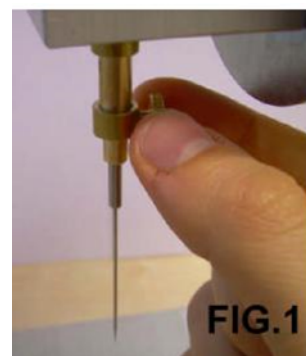

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	9/10	03/2009

Regulate the remaining height of the needle or cone so that the tip is skimming the surface of the sample. Turn the **A10** knob to regulate it.

Slowly lower the beam of the electronic meter so that its lower end is in contact with the upper spherical point of the **A13** penetration beam.

Tighten the **A12** knob; reset the numerical value on the electronic meter.

5.04 SWITCHING THE APPLIANCE ON

Press the **A4** key to start penetration.

5.05 TEST START UP

Before using the appliance regularly check it is working correctly by carrying out at least one complete empty cycle according to the previous instructions.

Should there be any problem consult the chapter "DIAGNOSTICS".

If the instructions in this manual do not provide the solution to the problem, contact Sales Assistance.

5.06 PRACTICAL USAGE EXAMPLE

Here follows an "example procedure" for an inexperienced operator to carry out a complete test. The experience of the operator will enable him to optimise use of the equipment according to his needs.

Consult the UNI EN1426 standard before starting the test.

1. Regulation of the base position – See the chapter :**REGULATION OF THE LEVEL OF THE BASE**
2. Equip and prepare the instrument – See the chapter : **SETTING UP – SAMPLE POSITIONING**
3. Push the button **A4** and keep on pushing it for at least 5 seconds. This is the necessary time to allow the penetration into the specimen.
4. After 5 seconds the position reached by the needle or the cone is automatically blocked and the penetration can now be measured; gently push the beam of the electronic meter down until it in contact with the upper spherical end of the penetration beam **A13**.
5. Record the value shown.

Chapter 6 MAINTENANCE

6.01 ORDINARY MAINTENANCE



DANGER WARNING

Do not perform maintenance – interventions on the machine which have not been quoted and described in this instructions manual without first contacting the manufacturer.
Periodically clean all machine parts and oil the unpainted parts in order to preserve the machine and its efficiency.
Avoid the use of solvents which damage paint and parts in synthetic material.

6.02 EXTRAORDINARY MAINTENANCE

For extraordinary maintenance operations refer directly to the Manufacturer.

6.03 AUTHORISED MAINTENANCE CENTRES

For information on the nearest authorised help centre it is essential to contact the manufacturer.

Chapter 7 GUIDE TO RECOGNISING DAMAGE AND ANOMALIES

This chapter presents and discusses all the simple problems which could occur during machine use.


The appropriately qualified, professional personnel must carry out all the maintenance procedures, check and control, as well as all the repair operations on parts of the machine or the electrical system.

Contact Technical Sales Assistance for any other problem not listed on the previous table or should the malfunctioning persist after the intervention of the operator in accordance with the previously mentioned courses of action.

Rev.	Descrizione	Redatto/Gestito	Approvato	Cod.Ident.	Pagine	Data Em.
02	Manuale Istruzioni	Ufficio Tecnico	Resp.Tecnico	B056-01KIT.M01.EN.02	10/10	03/2009

PROBLEM	POSSIBLE CAUSE	REMEDY
The electronic meter won't switch on or show the values correctly	Meter failure or power battery flat	Contact Technical Assistance.

Chapter 8 SPARE PARTS

	WARNING DANGER	Only original spare parts can be used. Use of unoriginal spare parts exempts the manufacturer from all responsibility. Procedures for substitution of spare parts will be provided by the manufacturer along with the part. For spare parts contact the manufacturer's Sales Service department.
---	---------------------------	---

SUGGESTED SPARE PART: PENETRATION ROD A13

Chapter 9 INACTIVITY

Ensure all machine parts are in safe working order before operating it again should the machine be inactive for a long period of time. When in doubt contact the Manufacturer.

Chapter 10 DECOMMISSIONING THE MACHINE

Should it be decided that the machine is to be no longer used, proceed as follows:

- Disconnect the electrical supply network by removing the connecting cable therefore making it unusable.
- Make the potential sources of danger harmless, such as sharp or protruding parts.
- Dismantle the machine; divide it into similar parts and dispose of according to the standards in force.

Recycling notice for the disposal of electrical and electronic devices



This symbol, shown on the device or on the package and/or the documentation, suggests that the device should not be disposed together with other home garbage at the end of its life cycle. To avoid further environment, or health-care damage, caused by the unsuitable disposal of garbage, the user should separate this device from other different types of garbage and recycle it in responsibly to avoid the reuse of material resources. Users must take care at the disposal of the equipment by taking it to the nearest recycling site for appropriate recycling treatment for electrical and electronic devices.

Gathering and

Recycling deplete devices allow the preservation of natural resources and grant them the adequate treatment by respecting health and environment.

For further information on your local recycling site please contact your local council or city waste treatment department. The developer, as producer of electrical and electronic devices, will provide to finance the recycling and treatment services for deplete devices that will come back through these recycling sites, according to the local statement.